


Astec P-CAP™ and P-CAP™-DP

Polycyclic amine polymer stationary phases
for chiral HPLC

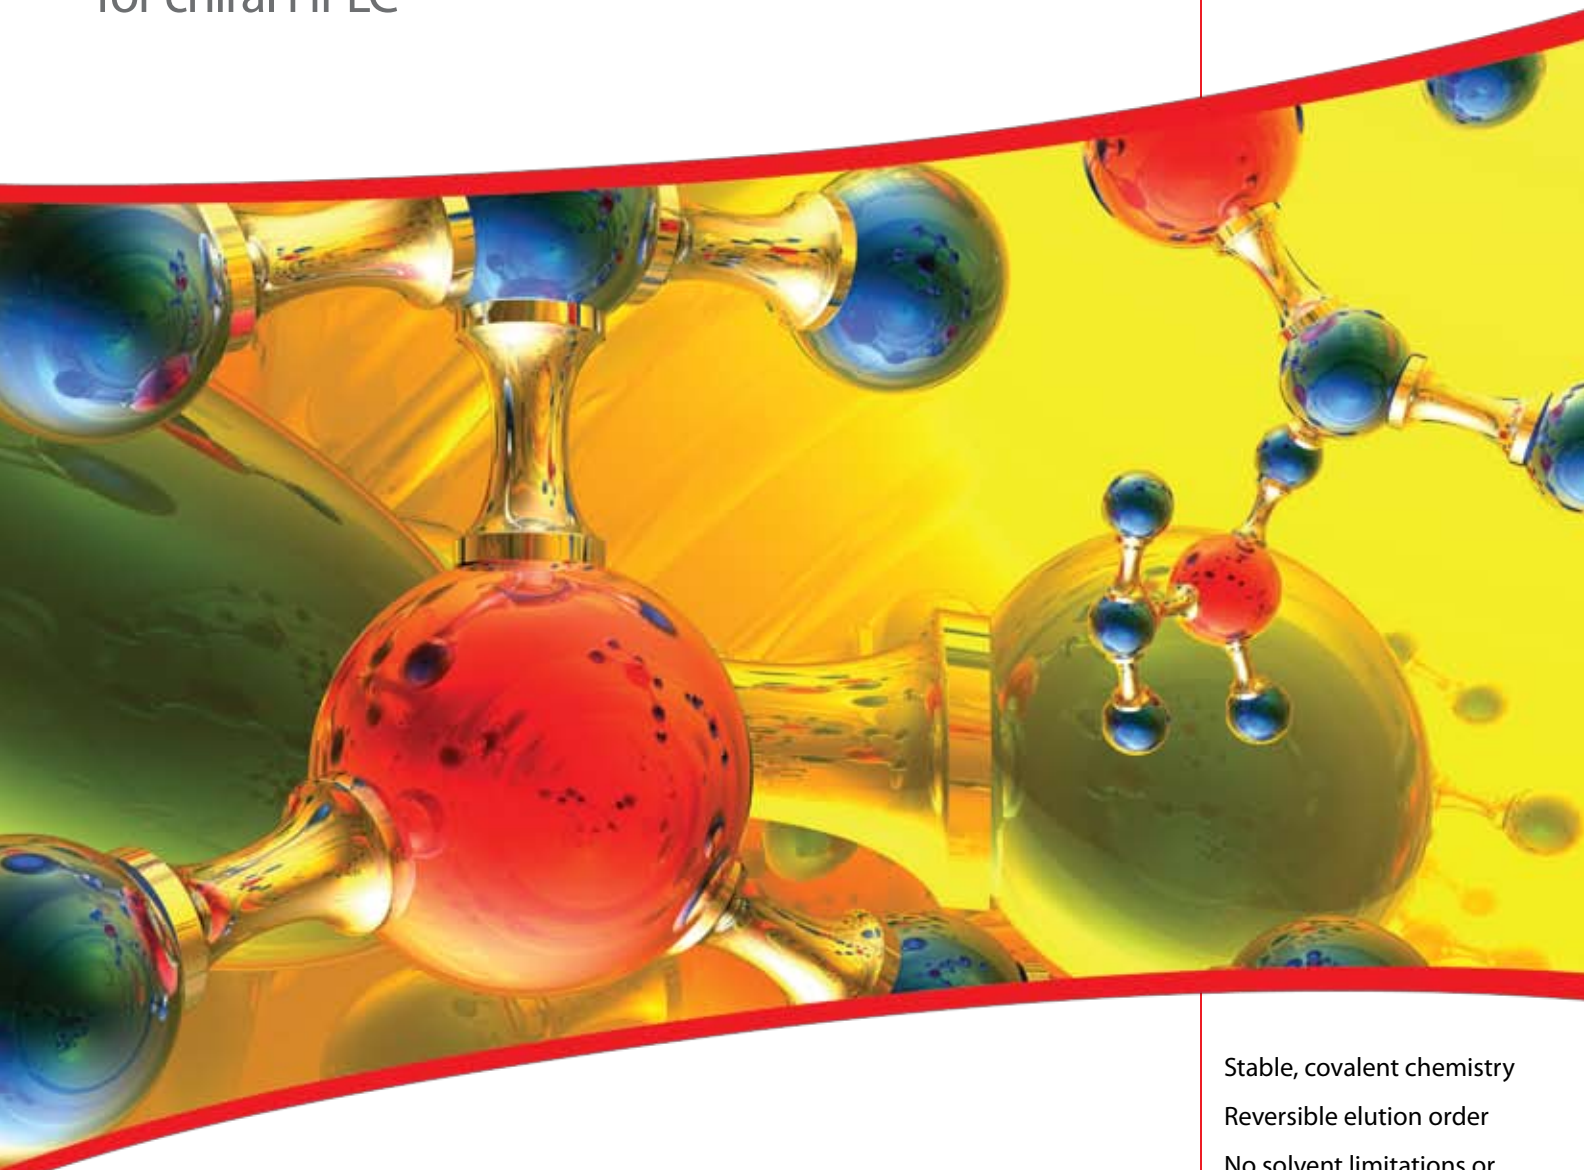

Stable, covalent chemistry

Reversible elution order

No solvent limitations or
memory effects

High capacity for prepara-
tive applications

MS and SFC-compatible

Chiral HPLC for Chemists: Ultimate Solvent Choice with High Capacity Using Astec's P-CAP and P-CAP-DP

Useful for chiral HPLC and SFC separations, Astec P-CAP and P-CAP-DP polymeric chiral stationary phases (CSPs) have a thin, ordered layer of chiral polymer covalently bonded to the silica surface. They offer high stability, high sample loadability, easy scale-up, and no memory effect.

Today's chiral HPLC columns too often give excellent enantioselectivity at the expense of solvent choice. Sample solubility and its link to preparative separations can mean that a compromise has to be reached between selectivity and solvent choice. Astec P-CAP and P-CAP-DP chiral HPLC columns have no solvent restrictions, so the user can select a solvent that provides optimum enantioselectivity and analyte solubility.

Astec P-CAP

- Bonded phase: Poly(trans-1,2-cyclohexanediyl-bis-acrylamide)
- Invented by Prof. Francesco Gasparrini (1), P-CAP is made from a diacryloyl-trans-1,2-diphenylethylenediamine polymerization, and utilizes hydrogen bonding and steric effects as enantiomer separation mechanisms.

Astec P-CAP-DP

- Bonded phase: Poly(diphenylethylenediamine-bis-acryloyl) or Poly-DPEDA
- Invented by Prof. Daniel Armstrong (2), Astec P-CAP-DP introduces phenyl rings to add π - π interactions, giving it one additional type of interaction compared to P-CAP. P-CAP-DP is less polar than P-CAP.

Solvent Choice and Reversal of Elution Order

The P-CAP and P-CAP-DP polyamide CSPs feature a thin, ordered polymer layer chemically bonded to 5 μm or 3.5 μm spherical silica using a patented radical polymerization. This gives the phases high permeability across the surface and, because they are synthetic, they can be identically manufactured in both R,R and S,S forms. This provides a predictable reversal of elution order in the same mobile phase (Figure 1).

The P-CAP phases have no solvent or additive memory effects, so the same column can be used in a number of different mobile phases without any detrimental effects. These phases form a new generation bridge between the traditional 'brush' type CSPs and the conventional polymeric phases.

Chiral method development is typically carried out either in normal phase (heptane/IPA or hexane/ethanol) or polar organic (acetonitrile/methanol) modes. For method optimization, a wide range of organic solvents can be used, from acetone to dichloromethane to dioxane, and many others. For acids and bases, the addition of 0.1% TFA often

Figure 1. Predictable Elution Order Reversal


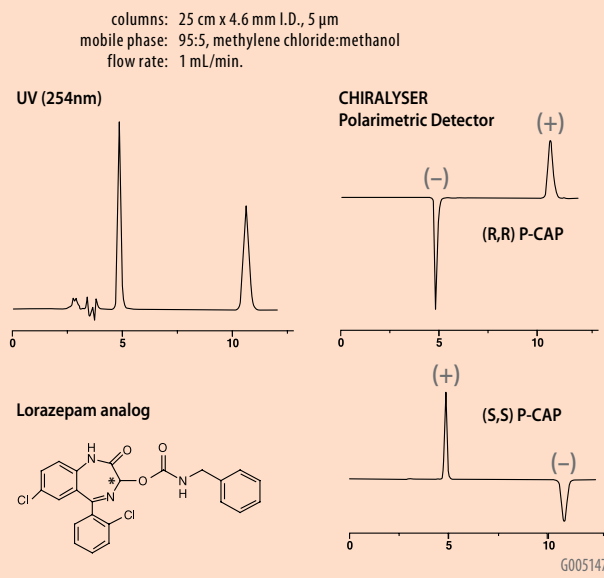


Figure 2. High-capacity Separations


Analyte: furoin

column: (R,R) P-CAP-DP, 25 cm x 4.6 mm I.D., 5 μm particles (25024AST)
mobile phase: 80:20, hexane:ethanol
flow rate: 1.0 mL/min.
temp.: 23 $^{\circ}\text{C}$
det.: UV at 235 nm
injection: (a) 2 μL at 4 mg/mL (8 μg total)
(b) 50 μL at 20 mg/mL (1000 μg total)

8 μg injection

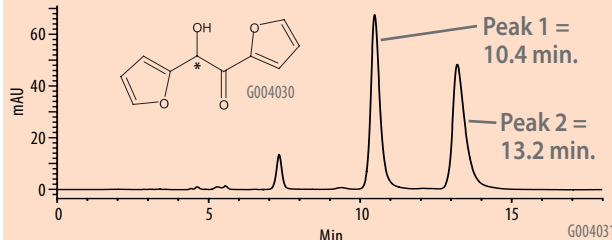

1000 μg injection

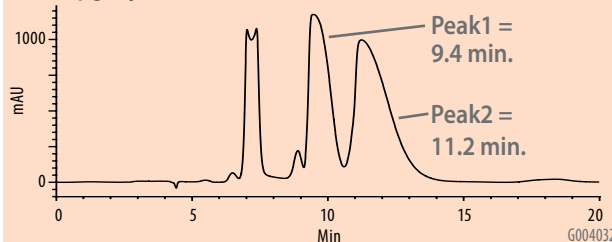

increases resolution and efficiency and decreases retention times. There are no known limitations on the kind of solvents that can be used with these phases. For MS detection, volatile acids and buffers such as ammonium acetate can be added to enhance peak efficiency or to enhance ionization when needed.

High Capacity for Preparative HPLC

Solvent flexibility and high loading capacity make P-CAP and P-CAP-DP CSPs ideal for analytical, preparative and process scale separations. The separation of fuoin enantiomers is shown in Figure 2 using an analytical 25 cm x 4.6 mm Astec (R,R) P-CAP-DP column and mobile phase of 80:20 hexane:ethanol. Excellent separation is demonstrated with an injection of 8 µg of the fuoin racemate. Increasing the load to 1 mg on this analytical column demonstrates the phase's high loading capacity.

MS-Compatible Operation

Astec P-CAP and P-CAP-DP operate in mobile phases that are amenable to MS-detection. Salt and/or acetic acid can be added to improve efficiency or enhance ionization and detection (Figure 3).

Applications

Astec P-CAP CSPs have been used for a wide variety of molecular types and are ideal for medium to high polarity compounds. The mechanism of separation is either through hydrogen bonding for P-CAP, or through both hydrogen bonding (donor and acceptor) with additional π - π interaction for the P-CAP-DP. Both also use dipole-dipole and steric interactions. Examples of the separations completed to date are shown in Table 1.

Table 1. Examples of P-CAP and P-CAP-DP Application Areas

Hydroxycarboxylic acids	Benzene sulfonamides
Alcohols	Binaphthols
Sulfoxides	Benzodiazepines
Esters	Phosphonic acids
Amides	Bis-Sulfones
N-blocked amino acids	Chromemones

Complementary to Other Astec CSPs


Astec P-CAP and P-CAP-DP are complementary to Astec CHIROBIOTIC, CYCLOBOND and the polysaccharide-based CSPs. We suggest you incorporate them into your chiral column screening protocol.

Figure 3. Improved Analytical Separation with MS-Compatible Mobile Phases

column: (R,R) P-CAP, 25 cm x 4.6 mm I.D., 5 µm particles (31024AST)
 flow rate: 1.0 mL/min.
 temp.: 25 °C
 det.: UV @ 254 nm


Separation of 1,1'-Bi-2-naphthol

mobile phase: 95:5:10 mM ammonium acetate:methanol:acetate

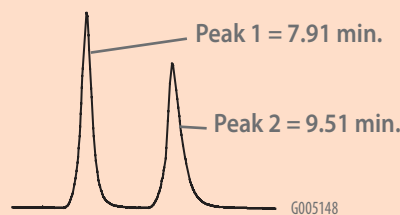


Oxazepam

mobile phase: 70:30:20 mM ammonium acetate:methanol:acetate

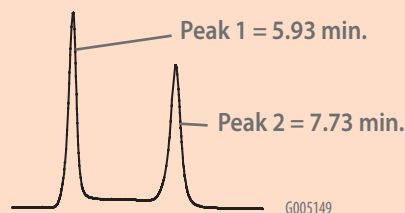

Lorazepam

mobile phase: 70:30:20 mM ammonium acetate:methanol:acetate

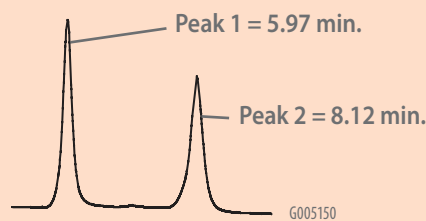

Summary

Astec P-CAP and P-CAP-DP are rugged chiral HPLC phases, experience no memory effects, and can be run in a wide variety of solvents with speed and high efficiencies. For preparative applications, a combination of wide solvent choice and high capacity make them ideal for large-scale purification.

References

- 1) New hybrid polymeric liquid chromatography chiral stationary phase prepared by surface initiated polymerization. Gasparrini, F.; Misiti, D.; Rompietti, R.; Villani, C. J Chromatogr, A. (2005), 1064(1), 25-38.
- 2) Chromatographic evaluation of poly(trans-1,2-cyclohexanediyl-bisacrylamide) as a chiral stationary phase for HPLC. Zhong, Qiqing; Han, Xinxin; He, Lingfeng; Beesley, Thomas E.; Trahanovsky, Walter S.; Armstrong, Daniel W. Department of Chemistry, Iowa State University, Ames, IA, USA. Journal of Chromatography, A (2005), 1066(1-2), 55-70.

Ordering Information

Particle Size (µm)	Length (cm)	I.D. (mm)	Cat. No.
Astec (R,R) P-CAP			
3.5	5	4.6	30021AST
3.5	10	4.6	30022AST
3.5	15	4.6	30023AST
5	5	4.6	31021AST
5	10	2.1	31018AST
5	10	4.6	31022AST
5	15	2.1	31019AST
5	15	4.6	31023AST
5	25	2.1	31020AST
5	25	4.6	31024AST
5	25	10	31034AST
5	25	21.2	31044AST
10	25	4.6	31124AST
Guards*			
5	2	1	31101AST
5	2	4	31100AST
Astec (S,S) P-CAP			
3.5	5	4.6	32021AST
3.5	10	4.6	32022AST
3.5	15	4.6	32023AST
5	5	4.6	33021AST
5	10	2.1	33018AST
5	10	4.6	33022AST
5	15	2.1	33019AST
5	15	4.6	33023AST
5	25	2.1	33020AST
5	25	4.6	33024AST
5	25	10	33034AST
5	25	21.2	33044AST
10	25	4.6	33124AST
Guards*			
5	2	1	33101AST
5	2	4	33100AST

Particle Size (µm)	Length (cm)	I.D. (mm)	Cat. No.
Astec (R,R) P-CAP-DP			
3.5	15	4.6	34023AST
5	15	2.1	35019AST
5	15	4.6	35023AST
5	25	4.6	35024AST
5	25	10	35034AST
5	25	21.2	35044AST
Guards*			
5	2	4	35100AST
Astec (S,S) P-CAP-DP			
3.5	15	4.6	36023AST
5	15	2.1	37019AST
5	15	4.6	37023AST
5	25	4.6	37024AST
5	25	10	37034AST
5	25	21.2	37044AST
Guards*			
5	2	4	37100AST
*Guard Column Holders			
Guard Holders for 4 mm I.D. cartridges (holder not required for 1 mm I.D. guards)			21150AST

Visit sigma-aldrich.com/chiral to see our complete offering of chiral chemistry, separation products, and services.

CHIROBIOTIC, CYCLOBOND and P-CAP are trademarks of Sigma-Aldrich Biotechnology LP

*Accelerating Customers'
Success through Innovation and
Leadership in Life Science,
High Technology and Service*

Order/Customer Service (800) 325-3010 • Fax (800) 325-5052
Technical Service (800) 325-5832 • sigma-aldrich.com/techservice
Development/Custom Manufacturing Inquiries **SAFC® (800) 244-1173**
Safety-related Information sigma-aldrich.com/safetycenter

World Headquarters
 3050 Spruce St.
 St. Louis, MO 63103
 (314) 771-5765
sigma-aldrich.com

©2010 Sigma-Aldrich Co. All rights reserved. SIGMA, SAFC, SIGMA-ALDRICH, ALDRICH, FLUKA, and SUPELCO are trademarks belonging to Sigma-Aldrich Co. and its affiliate Sigma-Aldrich Biotechnology, LP. Sigma brand products are sold through Sigma-Aldrich, Inc. Sigma-Aldrich, Inc. warrants that its products conform to the information contained in this and other Sigma-Aldrich publications. Purchaser must determine the suitability of the product(s) for their particular use. Additional terms and conditions may apply. Please see reverse side of the invoice or packing slip.

MNN
T410060